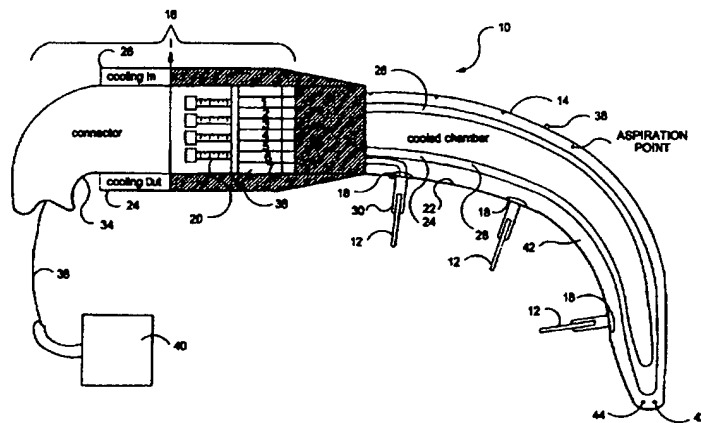


**PCT**WORLD INTELLECTUAL PROPERTY ORGANIZATION  
International Bureau

## INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

<b>(51) International Patent Classification 6 :</b> A61B 17/39, A61N 1/40, 5/04		<b>A1</b>	<b>(11) International Publication Number:</b> WO 97/30647
			<b>(43) International Publication Date:</b> 28 August 1997 (28.08.97)
<b>(21) International Application Number:</b> PCT/US97/02834		<b>(81) Designated States:</b> AL, AM, AT, AU, AZ, BA, BB, BG, BR, BY, CA, CH, CN, CU, CZ, DE, DK, EE, ES, FI, GB, GE, HU, IL, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MD, MG, MK, MN, MW, MX, NO, NZ, PL, PT, RO, RU, SD, SE, SG, SI, SK, TJ, TM, TR, TT, UA, UG, US, UZ, VN, ARIPO patent (KE, LS, MW, SD, SZ, UG), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, CH, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, ML, MR, NE, SN, TD, TG).	
<b>(22) International Filing Date:</b> 24 February 1997 (24.02.97)			
<b>(30) Priority Data:</b> 08/606,195 23 February 1996 (23.02.96) US 08/642,053 3 May 1996 (03.05.96) US			
<b>(71) Applicant (for all designated States except US):</b> SOMNUS MEDICAL TECHNOLOGIES, INC. [US/US]; 995 Benicia Avenue, Sunnyvale, CA 94086 (US).		<b>Published</b> <i>With international search report.</i> <i>Before the expiration of the time limit for amending the claims and to be republished in the event of the receipt of amendments.</i>	
<b>(71)(72) Applicant and Inventor:</b> EDWARDS, Stuart, D. [US/US]; 658 Westridge Drive, Portola Valley, CA 94028 (US).			
<b>(74) Agent:</b> DAVIS, Paul; Wilson Sonsini Goodrich & Rosati, 650 Page Mill Road, Palo Alto, CA 94304-1050 (US).			

**(54) Title:** APPARATUS AND METHOD FOR TREATING AIRWAY INSUFFICIENCY IN THE LARYNGEAL/ORAL CAVITY REGION BY ELECTROMAGNETIC ENERGY**(57) Abstract**

An ablation apparatus is provided which ablates at least a portion of an interior of a body structure while reducing a swelling response in the body structure. The apparatus provides a catheter including a catheter tissue interface surface and a port formed in the catheter tissue interface surface. An electrode is at least partially positioned in the interior of the catheter and configured to be advanced and retracted in and out of the port. The electrode includes an electrode electromagnetic energy delivery surface. A cooling element includes a cooling medium inlet conduit and a cooling medium exit conduit, both extending through an interior of the catheter forming at least a partial cooled catheter tissue interface surface. The electrode electromagnetic energy delivery surface is thermally isolated from the cooling element. An electrode advancement and retraction device is at least partially positioned in the interior of the catheter. A cable is coupled to the electrode.

**FOR THE PURPOSES OF INFORMATION ONLY**

Codes used to identify States party to the PCT on the front pages of pamphlets publishing international applications under the PCT.

AM	Armenia	GB	United Kingdom	MW	Malawi
AT	Austria	GE	Georgia	MX	Mexico
AU	Australia	GN	Guinea	NE	Niger
BB	Barbados	GR	Greece	NL	Netherlands
BE	Belgium	HU	Hungary	NO	Norway
BF	Burkina Faso	IE	Ireland	NZ	New Zealand
BG	Bulgaria	IT	Italy	PL	Poland
BJ	Benin	JP	Japan	PT	Portugal
BR	Brazil	KE	Kenya	RO	Romania
BY	Belarus	KG	Kyrgyzstan	RU	Russian Federation
CA	Canada	KP	Democratic People's Republic of Korea	SD	Sudan
CF	Central African Republic	KR	Republic of Korea	SE	Sweden
CG	Congo	KZ	Kazakhstan	SG	Singapore
CH	Switzerland	LJ	Liechtenstein	SI	Slovenia
CJ	Côte d'Ivoire	LK	Sri Lanka	SK	Slovakia
CM	Cameroon	LR	Liberia	SN	Senegal
CN	China	LT	Lithuania	SZ	Swaziland
CS	Czechoslovakia	LU	Luxembourg	TD	Chad
CZ	Czech Republic	LV	Latvia	TG	Togo
DE	Germany	MC	Monaco	TJ	Tajikistan
DK	Denmark	MD	Republic of Moldova	TT	Trinidad and Tobago
EE	Estonia	MG	Madagascar	UA	Ukraine
ES	Spain	ML	Mali	UG	Uganda
FI	Finland	MN	Mongolia	US	United States of America
FR	France	MR	Mauritania	UZ	Uzbekistan
GA	Gabon			VN	Viet Nam

APPARATUS AND METHOD FOR TREATING AIRWAY INSUFFICIENCY IN THE LARINGEAL/ORAL  
CAVITY REGION BY ELECTROMAGNETIC ENERGY

Cross-Reference to Related Applications

5           This application is a continuation-in-part application of U.S. Patent  
Application No. 08/606,195, filed February 23, 1996, entitled "Method for  
Treatment of Airway Obstructions", which cross-references U.S. Patent  
Application No. 08/516,781 filed August 18, 1995, entitled "Ablation Apparatus  
and System for Removal of Soft Palate Tissue", having named inventors Stuart  
10   D. Edwards, Edward J. Gough and David L. Douglass, which is a continuation-  
in-part of U.S. Application No. 08/239,658, filed May 9, 1994 entitled "Method  
for Reducing Snoring by RF Ablation of the Uvula", and is related to Attorney  
Docket No. SOMN 1009CIP3, entitled "Method and Apparatus for Treatment  
of Air Way Obstructions" filed concurrent with this application, all incorporated  
15   by reference herein.

BACKGROUND OF THE INVENTION

Field of the Invention

          This invention relates to a method for maintaining upper airway patency  
in human patients, and more particularly to a method which utilizes  
20   electromagnetic energy to debulk selected sections of the tongue and/or lingual  
tonsil without damaging the hypoglossal nerve.

Description of Related Art

          Sleep-apnea syndrome is a medical condition characterized by daytime  
hypersomnolence, morning arm aches, intellectual deterioration, cardiac  
25   arrhythmias, snoring and thrashing during sleep. It is caused by frequent  
episodes of apnea during the patient's sleep. The syndrome is classically  
subdivided into two types. One type, termed "central sleep apnea syndrome", is  
characterized by repeated loss of respiratory effort. The second type, termed

obstructive sleep apnea syndrome, is characterized by repeated apneic episodes during sleep resulting from obstruction of the patient's upper airway or that portion of the patient's respiratory tract which is cephalad to, and does not include, the larynx.

5           Treatment thus far includes various medical, surgical and physical measures. Medical measures include the use of medications such as protriptyline, medroxyprogesterone, acetazolamide, theophylline, nicotine and other medications in addition to avoidance of central nervous system depressants such as sedatives or alcohol. The medical measures above are sometimes helpful  
10 but are rarely completely effective. Further, the medications frequently have undesirable side effects.

          Surgical interventions have included uvulopalatopharyngoplasty, tonsillectomy, surgery to correct severe retrognathia and tracheostomy. In one procedure the jaw is dislodged and pulled forward, in order to gain access to the  
15 base of the tongue. These procedures may be effective but the risk of surgery in these patients can be prohibitive and the procedures are often unacceptable to the patients.

          Physical measures have included weight loss, nasopharyngeal airways, nasal CPAP and various tongue retaining devices used nocturnally. These  
20 measures may be partially effective but are cumbersome, uncomfortable and patients often will not continue to use these for prolonged periods of time. Weight loss may be effective but is rarely achieved by these patients.

          In patients with central sleep apnea syndrome, phrenic nerve or diaphragmatic pacing has been used. Phrenic nerve or diaphragmatic pacing  
25 includes the use of electrical stimulation to regulate and control the patient's diaphragm which is innervated bilaterally by the phrenic nerves to assist or support ventilation. This pacing is disclosed in *Direct Diaphragm Stimulation* by J. Mugica et al. PACE vol. 10 Jan-Feb. 1987, Part II, *Preliminary Test of a Muscular Diaphragm Pacing System on Human Patients* by J. Mugica et al.  
30 from *Neurostimulation: An Overview* 1985 pp. 263-279 and *Electrical*

*Activation of Respiration* by Nochomovitz IEEE Eng. in Medicine and Biology; June, 1993.

5 However, it was found that many of these patients also have some degree of obstructive sleep apnea which worsens when the inspiratory force is augmented by the pacer. The ventilation induced by the activation of the diaphragm also collapses the upper airway upon inspiration and draws the patient's tongue inferiorly down the throat choking the patient. These patients then require tracheostomies for adequate treatment.

10 A physiological laryngeal pacemaker as described in *Physiological Laryngeal Pacemaker* by F. Kaneko et al. from Trans Am Soc Artif Intern Organs 1985 senses volume displaced by the lungs and stimulates the appropriate nerve to open the patient's glottis to treat dyspnea. This apparatus is not effective for treatment of sleep apnea. The apparatus produces a signal proportional in the displaced air volume of the lungs and thereby the signal  
15 produced is too late to be used as an indicator for the treatment of sleep apnea. There is often no displaced air volume in sleep apnea due to obstruction.

One measure that is effective in obstructive sleep apnea is tracheostomy. However, this surgical intervention carries considerable morbidity and is aesthetically unacceptable to many patients. Other surgical procedures include  
20 pulling the tongue as forward as possible and surgically cutting and removing sections of the tongue and other structures which can close off the upper airway passage.

25 There is a need for a method and apparatus to treat airway obstruction disorders. There is a further need for a method and apparatus which delivers sufficient electromagnetic energy to an interior of a body structure, including but not limited to the tongue, to treat airway obstruction disorders while reducing a swelling of an exterior surface of the body structure.

### SUMMARY OF THE INVENTION

Accordingly, an object of the invention is to provide a method and apparatus to treat airway obstructions.

5 Another object of the invention is to provide a method and apparatus for ablating an interior of a body structure while reducing a swelling of an exterior surface of the body structure.

10 Still another object of the invention is to provide a method and apparatus for ablating an interior of a body structure by providing a cooled catheter tissue interface surface that is cooled sufficient to reduce a swelling of the body structure.

A further object of the invention is to provide a method and apparatus for ablating an interior of the tongue while reducing a swelling of an exterior surface of the tongue.

15 Yet another object of the invention is to provide a method and apparatus for ablating an interior of the tongue while providing sufficient cooling to an exterior surface of the tongue in order to reduce swelling of the exterior surface.

20 These and other objects of the invention are achieved in an ablation apparatus which ablates at least a portion of an interior of a body structure while reducing a swelling response in the body structure. The apparatus provides a catheter including a catheter tissue interface surface and a port formed in the catheter tissue interface surface. An electrode is at least partially positioned in the interior of the catheter and configured to be advanced and retracted in and out of the port. The electrode includes an electrode electromagnetic energy delivery surface. A cooling element includes a cooling medium inlet conduit and  
25 a cooling medium exit conduit, both extending through an interior of the catheter forming at least a partial cooled catheter tissue interface surface. The electrode electromagnetic energy delivery surface is thermally isolated from the cooling element. An electrode advancement and retraction device is at least partially positioned in the interior of the catheter. A cable is coupled to the electrode.

In one embodiment of the invention, a method for treating airway obstructions provides an ablation apparatus. The ablation apparatus includes a catheter with a catheter tissue interface surface, an electrode at least partially positioned in an interior of the catheter and advanceable and retractable to and from the catheter into an interior of a body structure, and a means for cooling the catheter tissue interface surface. The electrode is advanced from the interior of the catheter through a body structure external surface into the interior of the body structure. Sufficient electromagnetic energy is delivered from the electrode into the interior of the body structure to ablate a portion of the interior of the body structure. The catheter tissue interface surface is cooled sufficiently to reduce a swelling of the body structure external surface. The electrode is retracted from the interior of the body structure.

The catheter tissue interface surface can be cooled to a temperature of 10 to 30 degrees C. The electrode may be hollow and coupled to an infusion medium source. An insulation sleeve can be positioned in a surrounding relationship to at least a portion of an exterior surface of the electrode. One or more electrodes may be introduced through the catheter. Additionally, one or more sensors can be positioned at various locations of the ablation apparatus including at a distal end of the electrode, at an exterior surface of the electrode, at a distal end of the insulation sleeve or at the catheter tissue interface surface. A variety of different electromagnetic energy sources can be coupled to the electrode including but not limited to RF and microwave sources.

In one embodiment, the body structure is the tongue. The electrode is introduced through the tongue's ventral surface, dorsal surface or the dorsum surface. Sufficient cooling is provided to reduce a swelling of the exterior surface of a tongue following delivery of electromagnetic energy to an interior of the tongue by at least fifty percent.

#### **BRIEF DESCRIPTION OF THE FIGURES**

Figure 1(a) is a cross-sectional view of an ablation apparatus used with the present invention.

Figure 1(b) is a perspective of the ablation apparatus of the present invention illustrating a catheter tissue interface surface.

5           Figure 2 is cross-sectional view illustrating the catheter and connector of the ablation apparatus shown in Figure 1(a).

Figure 3 is a perspective view of the connector illustrated in Figure 1(a).

Figure 4 is a perspective view of a needle electrode associated with the ablation apparatus illustrated in Figure 1(a).

10           Figure 5 is a perspective view of a flexible needle electrode utilized with the methods of the present invention.

Figure 6 illustrates the creation of ablation zones with the ablation apparatus shown in Figure 1(a).

Figure 7 is a cross-sectional view of the tongue with the mouth closed.

15           Figure 8 is a cross-sectional view of the tongue with the mouth open.

Figure 9 is a perspective view of the tongue.

Figure 10 is a perspective view of the dorsum of the tongue.

Figure 11 is a cross-sectional view of the tongue.

20           Figure 12 is a cross-sectional view of the tongue illustrating the location of the hypoglossal nerves and the creation of an ablation zone.

Figure 13 is a cross-sectional view of the tongue illustrating a plurality of ablation zones.

Figure 14 is a perspective view of the ventral surface of the tongue.

Figure 15 is a cross-sectional view of the tongue.

25           Figure 16 is a block diagram of a feedback control system useful with the methods of the present invention.

Figure 17 is a block diagram illustrating an analog amplifier, analog multiplexer and microprocessor used with the feedback control system of Figure 16.



Figure 18 is a block diagram of a temperature/impedance feedback system that can be used to control cooling medium flow rate through the catheter of Figure 1.

#### DETAILED DESCRIPTION

5 Referring to Figures 1(a), 1(b) and 2, an ablation apparatus 10 for debulking the tongue, lingual tonsils, and/or adenoids is illustrated. Ablation apparatus 10 can be positioned so that one or more electrodes 12 are introduced into an interior of the tongue through a surface of the tongue. Ablation apparatus 10 may include atraumatic intubation with or without visualization,  
10 provide for the delivery of oxygen or anesthetics, and can be capable of suctioning blood or other secretions. It will be appreciated that ablation apparatus 10 is used to treat a variety of different obstructions in the body where passage of gas is restricted. One embodiment is the treatment of sleep apnea using electrodes 12 to ablate selected portions of the tongue, lingual tonsils and/or adenoids by the use of RF, microwave, and the like. In this regard,  
15 ablation apparatus 10 can be used to ablate targeted masses including but not limited to the tongue, tonsils, turbinates, soft palate tissues, hard tissue and mucosal tissue. In one embodiment, ablation apparatus 10 is used to ablate an interior region of the tongue, causing it to become debulked in order to increase  
20 the cross-sectional area of the airway passage.

Prior to debulking the tongue, a presurgical evaluation may be performed including a physical examination, fiber optic pharyngoscopy, cephalometric analysis and polygraphic monitoring. The physical examination emphasizes the evaluation of the head and neck. It also includes a close examination of the nasal  
25 cavity to identify obstructing deformities of the septum and turbinate; oropharyngeal obstruction from a long, redundant soft palate or hypertrophic tonsils; and hypopharyngeal obstruction from a prominent base of the tongue.

Ablation apparatus 10 includes a catheter 14, a handle 16, one or more electrodes 12 extending from different ports 18 formed along a longitudinal

surface of catheter 14, or from a distal end of electrode 12. An electrode advancement and retraction device 20 is provided. Cabling is coupled to electrodes 12.

Electrodes 12 are at least partially positioned in an interior of catheter 14. Each electrode 12 is advanced and retracted through a port 18 formed in an exterior surface of catheter 14. Electrode advancement and retraction device advances electrodes 12 out of catheter 14, into an interior of a body structure and retracted back into catheter 14. Although the body structure can be any number of different structures, the body structure will hereafter be referred to as the tongue. Electrodes 12 pierce an exterior surface of the tongue and are directed to an interior region of the tongue. Sufficient electromagnetic energy is delivered by electrodes 12 to the interior of the tongue to cause the tongue to become sufficiently ablated and debulked. Electrodes 12 can be hollow to receive a variety of different infusion mediums, including but not limited to saline. Electrodes 12 may be limited in the distance that they can be advanced into the tongue. This is achieved with an insulation sleeve, a structure located on electrodes 12 which limits their advancement, or a structure coupled to catheter which limits the advancement of electrodes 12, such as a stop and the like.

Electrodes 12 can include a central lumen for receiving a variety of fluids that can be introduced into the interior of the tongue, as well as a plurality of fluid delivery ports. One suitable fluid is an electrolytic solution. Instead of direct contact with tissue and electrode 12 for the delivery of thermal energy, a cooled electrolytic solution can be used to deliver the thermal energy to the tissue. The electrolytic solution may be cooled in the range of about 30 to 55 degrees C.

Catheter 14 includes a catheter tissue interface surface 22, a cooling medium inlet conduit 24 and a cooling medium exit conduit 26 extending through an interior of catheter 14. Ports 18 are formed in the exterior of catheter 14, and are preferably formed on catheter tissue interface surface 22. Ports 18 are isolated from a cooling medium flowing in inlet and outlet conduits

24 and 26. Cooling medium inlet and exit conduits 24 and 26 are configured to provide a cooled section of catheter tissue interface surface 22 of at least 1 to 2 cm<sup>2</sup>. More preferably, the cooled section of catheter tissue interface surface 22 is at least equal to the cross-sectional diameter of the underlying zone of ablation.

The size of the cooled section of catheter tissue interface surface 22 varies for each patient. The size is sufficient enough to minimize swelling of the tongue following the delivery of electromagnetic energy. The reduction of swelling can be 50% or greater, 75% or greater, and 90% and greater. The amount of cooling provided is sufficient to enable the patient to return home shortly after the debulking procedure is performed, and not run the risk of choking on the tongue. It has been found that by providing a sufficient level of cooling over a relatively large area, the amount of ablation in an interior region of the tongue is enhanced. By providing a sufficiently large enough cooled section of catheter tissue interface surface 22, an adenomas response is minimized.

An electromagnetic energy delivery surface 30 of electrode 12 can be adjusted by inclusion of an adjustable or non-adjustable insulation sleeve 32 (Figures 3, 4, and 5). Insulation sleeve 32 can be advanced and retracted along the exterior surface of electrode 12 in order to increase or decrease the length of the electromagnetic energy delivery surface 30. Insulation sleeve 32 can be made of a variety of materials including but not limited to nylon, polyimides, other thermoplastics and the like. The size of electromagnetic energy delivery surface 30 can be varied by other methods including but not limited to creating a segmented electrode with a plurality of electrodes that are capable of being multiplexed and individually activated, and the like.

Handle 16 is preferably made of an insulating material. Electrodes 12 are made of a conductive material such as stainless steel. Additionally, electrodes 12 can be made of a shaped memory metal, such as nickel titanium, commercially available from Raychem Corporation, Menlo Park, California. In one

embodiment, only a distal end of electrode 12 is made of the shaped memory metal in order to effect a desired deflection. When introduced into the oral cavity, catheter 14 can be advanced until a patient's gag response is initiated. Catheter 14 is then retracted back to prevent patient's gagging. The distal end of electrode 12 can be semi-curved. The distal end can have a geometry to conform to an exterior of the tongue.

Catheter 14 can be malleable in order to conform to the surface of the tongue when a selected ablation target site is selected. An encapsulated soft metal, such as copper, or an annealed metal/plastic material can be used to form malleable catheter 14. All or a portion of catheter 14 may be malleable or made of a shaped memory metal.

For many applications it is desirable for a distal end 14' of catheter 14 to be deflectable. This can be achieved mechanically or with the use of memory metals. A steering wire, or other mechanical structure, can be attached to either the exterior or interior of distal end 14'. In one embodiment, a deflection knob located on handle 16 is activated by the physician causing a steering wire to tighten. This imparts a retraction of distal end 14', resulting in its deflection. It will be appreciated that other mechanical devices can be used in place of the steering wire. The deflection may be desirable for tissue sites with difficult access.

Handle 6 can comprise a connector 34 coupled to retraction and advancement device 20. Connector 34 provides a coupling of electrodes 12 to power, feedback control, temperature and/or imaging systems. An RF/temperature control block 36 can be included.

In one embodiment, the physician moves retraction and advancement device 20 in a direction toward a distal end of connector 34. Electrodes 12 can be spring loaded. When retraction and advancement device 20 is moved back, springs cause selected electrodes 12 to advance out of catheter 14.

One or more cables 38 couple electrodes 12 to an electromagnetic energy source 40. A variety of energy sources 40 can be used with the present

invention to transfer electromagnetic energy to the interior of a body structure, including but not limited to RF, microwave, ultrasound, coherent light and thermal transfer. Preferably, energy source 40 is a RF generator. When a RF energy source is used, the physician can activate RF energy source 40 by the use of a foot switch (not shown) coupled to RF energy source 40.

One or more sensors 42 may be positioned on an interior or exterior surface of electrode 12, insulation sleeve 32, or be independently inserted into the interior of the body structure. Sensors 42 permit accurate measurement of temperature at a tissue site in order to determine, (i) the extent of ablation, (ii) the amount of ablation, (iii) whether or not further ablation is needed, and (iv) the boundary or periphery of the ablated geometry. Further, sensors 42 prevent non-targeted tissue from being destroyed or ablated.

Sensors 42 are of conventional design, including but not limited to thermistors, thermocouples, resistive wires, and the like. Suitable sensors 42 include a T type thermocouple with copper constantene, J type, E type, K type, fiber optics, resistive wires, thermocouple IR detectors, and the like. It will be appreciated that sensors 42 need not be thermal sensors.

Sensors 42 measure temperature and/or impedance to permit ablation monitoring. This reduces damage to tissue surrounding the targeted ablation mass. By monitoring the temperature at various points within the interior of the body structure the periphery of ablation can be ascertained and it is possible to determine when the ablation is completed. If at any time sensor 42 determines that a desired ablation temperature is exceeded, then an appropriate feedback signal is received at energy source 40 and the amount of energy delivered is regulated.

Ablation apparatus 10 can include visualization capability including but not limited to a viewing scope, an expanded eyepiece, fiber optics, video imaging, and the like.

Additionally, ultrasound imaging can be used to position the electrodes 12 and/or determine the amount of ablation. One or more ultrasound

transducers 44 can be positioned in or on electrode 12, catheter 14, or on a separate device. An imaging probe may also be used internally or externally to the selected tissue site. A suitable imaging probe is Model 21362, manufactured and sold by Hewlett Packard Company. Each ultrasound transducer 44 is  
5 coupled to an ultrasound source (not shown).

With reference now to Figure 6 catheter 14 is shown as being introduced into the oral cavity and multiple RF electrodes 12 are advanced into the interior of the tongue creating different ablation zones 46. Ablation apparatus 10 can be operated in either bipolar or monopolar modes. In Figure 6, electrodes 12 are  
10 operated in the bipolar mode, creating sufficient ablation zones 46 to debulk the tongue without affecting the hypoglossal nerves and creating a larger airway passage. With this debulking, the back of the tongue moves in a forward direction away from the air passageway. The result is an increase in the cross-sectional diameter of the air passageway.

Ablation apparatus 10 can also be operated in the monopolar mode. A  
15 groundpad can be positioned in a convenient place such as under the chin. A single electrode 12 is positioned in the tongue to create a first ablation zone 46. Electrode 12 can then be retracted from the interior of the tongue, catheter 14 moved, and electrode 12 is then advanced from catheter 14 into another interior  
20 section of the tongue. A second ablation zone 46 is created. This procedure can be completed any number of times to form different ablation regions in the interior of the tongue. More than one electrode 12 can be introduced into the tongue and operated in the bipolar mode. Electrodes 12 are then repositioned in the interior of the tongue any number of times to create a plurality of connecting  
25 or non-connecting ablation zones 46.

Referring now to Figures 7 through 15, various anatomical views of the tongue and other structures are illustrated. The different anatomical structures are as follows: the genioglossus muscle, or body of the tongue is denoted as 48; the geniohyoid muscle is 50; the mylohyoid muscle is 52; the hyoid bone is 54;  
30 the tip of the tongue is 56; the ventral surface of the tongue is denoted as 58; the

dorsum of the tongue is denoted as 60; the inferior dorsal of the tongue is denoted as 62; the reflex of the vallecula is 64; the lingual follicles are denoted as 66; the uvula is 68; the adenoid area is 70; the lateral border of the tongue is 72; the circumvallate papilla is 74, the palatine tonsil is 76; the pharynx is 78; the  
5 redundant pharyngeal tissue is 80; the foramen cecum is 82; the hypoglossal nerve is 84, and the lingual frenum of the tongue is 86.

Dorsum 60 is divided into an anterior 2/3 and inferior dorsal 62. The delineation is determined by circumvallate papilla 74 and foramen cecum 82. Inferior dorsal 62 is the dorsal surface inferior to circumvallate papilla 74 and  
10 superior reflex of the vallecula 64. Reflex of the vallecula 64 is the deepest portion of the surface of the tongue contiguous with the epiglottis. Lingual follicles 66 comprise the lingual tonsil.

Catheter 14 can be introduced through the nose or through the oral cavity. Electrodes 12 can be inserted into an interior of the tongue through  
15 dorsum surface 60, inferior dorsal surface 62, ventral surface 58, tip 56 or geniohyoid muscle 50. Additionally, electrodes may be introduced into an interior of lingual follicles 66 and into adenoid area 70. Once electrodes 12 are positioned, insulation sleeve 32 may be adjusted to provided a desired electromagnetic energy delivery surface 30 for each electrode 12.

20 Ablation zones 46 are created without damaging hypoglossal nerves 84. This creates a larger air way passage and provides a treatment for sleep apnea.

In all instances, the positioning of electrodes 12, as well as the creation of ablation zones 46 is such that hypoglossal nerves 84 are not ablated or damaged. The ability to swallow and speak is not impaired.

25 Referring now to Figures 16 and 17 an open or closed loop feedback system couples sensors 42 to energy source 40. The temperature of the tissue, or of electrode 12 is monitored, and the output power of energy source 40 adjusted accordingly. The physician can, if desired, override the closed or open loop system. A microprocessor can be included and incorporated in the closed  
30 or open loop system to switch power on and off, as well as modulate the power.

The closed loop system utilizes a microprocessor 88 to serve as a controller, watch the temperature, adjust the RF power, look at the result, refeed the result, and then modulate the power.

5           With the use of sensors 42 and the feedback control system a tissue adjacent to RF electrodes 12 can be maintained at a desired temperature for a selected period of time without impeding out. Each RF electrode 12 is connected to resources which generate an independent output for each RF electrode 12. An output maintains a selected energy at RF electrodes 12 for a selected length of time.

10           Current delivered through RF electrodes 12 is measured by current sensor 90. Voltage is measured by voltage sensor 92. Impedance and power are then calculated at power and impedance calculation device 94. These values can then be displayed at user interface and display 96. Signals representative of power and impedance values are received by a controller 98.

15           A control signal is generated by controller 98 that is proportional to the difference between an actual measured value, and a desired value. The control signal is used by power circuits 100 to adjust the power output in an appropriate amount in order to maintain the desired power delivered at respective RF electrodes 12.

20           In a similar manner, temperatures detected at sensors 42 provide feedback for maintaining a selected power. The actual temperatures are measured at temperature measurement device 102, and the temperatures are displayed at user interface and display 96. A control signal is generated by controller 98 that is proportional to the difference between an actual measured  
25           temperature, and a desired temperature. The control signal is used by power circuits 100 to adjust the power output in an appropriate amount in order to maintain the desired temperature delivered at the respective sensor. A multiplexer can be included to measure current, voltage and temperature, at the numerous sensors 42, and energy can be delivered to RF electrodes 12 in  
30           monopolar or bipolar fashion.



Controller 98 can be a digital or analog controller, or a computer with software. When controller 98 is a computer it can include a CPU coupled through a system bus. On this system can be a keyboard, a disk drive, or other non-volatile memory systems, a display, and other peripherals, as are known in the art. Also coupled to the bus is a program memory and a data memory.

User interface and display 96 includes operator controls and a display. Controller 98 can be coupled to imaging systems, including but not limited to ultrasound, CT scanners, X-ray, MRI, mammographic X-ray and the like. Further, direct visualization and tactile imaging can be utilized.

The output of current sensor 90 and voltage sensor 92 is used by controller 98 to maintain a selected power level at RF electrodes 12. The amount of RF energy delivered controls the amount of power. A profile of power delivered can be incorporated in controller 98, and a preset amount of energy to be delivered can also be profiled.

Circuitry, software and feedback to controller 98 result in process control, and the maintenance of the selected power that is independent of changes in voltage or current, and are used to change, (i) the selected power, (ii) the duty cycle (on-off and wattage), (iii) bipolar or monopolar energy delivery, and (iv) infusion medium delivery, including flow rate and pressure. These process variables are controlled and varied, while maintaining the desired delivery of power independent of changes in voltage or current, based on temperatures monitored at sensors 42.

Current sensor 90 and voltage sensor 92 are connected to the input of an analog amplifier 104. Analog amplifier 104 can be a conventional differential amplifier circuit for use with sensors 42. The output of analog amplifier 104 is sequentially connected by an analog multiplexer 106 to the input of A/D converter 108. The output of analog amplifier 104 is a voltage which represents the respective sensed temperatures. Digitized amplifier output voltages are supplied by A/D converter 108 to microprocessor 88. Microprocessor 88 may be a type 68HCII available from Motorola. However, it will be appreciated that

any suitable microprocessor or general purpose digital or analog computer can be used to calculate impedance or temperature.

Microprocessor 88 sequentially receives and stores digital representations of impedance and temperature. Each digital value received by microprocessor 88 corresponds to different temperatures and impedances.

Calculated power and impedance values can be indicated on user interface and display 96. Alternatively, or in addition to the numerical indication of power or impedance, calculated impedance and power values can be compared by microprocessor 88 with power and impedance limits. When the values exceed predetermined power or impedance values, a warning can be given on user interface and display 96, and additionally, the delivery of RF energy can be reduced, modified or interrupted. A control signal from microprocessor 88 can modify the power level supplied by energy source 40.

Figure 18 illustrates a block diagram of a temperature/impedance feedback system that can be used to control cooling medium flow rate through catheter 14. Electromagnetic energy is delivered to electrode 12 by energy source 44, and applied to tissue. A monitor 110 ascertains tissue impedance, based on the energy delivered to tissue, and compares the measured impedance value to a set value. If the measured impedance exceeds the set value a disabling signal 112 is transmitted to energy source 40, ceasing further delivery of energy to electrode 12. If measured impedance is within acceptable limits, energy continues to be applied to the tissue. During the application of energy to tissue sensor 42 measures the temperature of tissue and/or electrode 12. A comparator 114 receives a signal representative of the measured temperature and compares this value to a pre-set signal representative of the desired temperature. Comparator 114 sends a signal to a flow regulator 116 representing a need for a higher cooling medium flow rate, if the tissue temperature is too high, or to maintain the flow rate if the temperature has not exceeded the desired temperature.

The foregoing description of a preferred embodiment of the invention has been presented for purposes of illustration and description. It is not intended to be exhaustive or to limit the invention to the precise forms disclosed. Obviously, many modifications and variations will be apparent to practitioners skilled in this art. It is intended that the scope of the invention be defined by the following claims and their equivalents.

What is claimed is:

**CLAIMS**

1. An apparatus for ablating at least a portion of an interior of a body structure, comprising:
- 5 a catheter including a catheter tissue interface surface and a port formed in the catheter tissue interface surface;
- an electrode at least partially positioned in the interior of the catheter and configured to be advanced and retracted in and out of the port, the electrode including an electrode electromagnetic energy delivery surface;
- 10 a cooling element including a cooling medium inlet conduit and a cooling medium exit conduit both extending through an interior of the catheter forming at least a partial cooled catheter tissue interface surface, wherein the electrode electromagnetic energy delivery surface is thermally isolated from the cooling element;
- 15 an electrode advancement and retraction device at least partially positioned in the interior of the catheter; and
- a cable coupled to the electrode.
2. The apparatus of claim 1, further comprising:
- two or more electrodes with a cooled tissue interface surface of at least 1 cm<sup>2</sup> for each electrode.
- 20 3. The apparatus of claim 1, wherein the cooling medium inlet and exit conduits are configured to cool the cooled catheter tissue interface surface to a temperature of 10 to 30 degrees C.
4. The apparatus of claim 1, wherein the electrode is hollow.
5. The apparatus of claim 4, further comprising:
- 25 an infusion medium source coupled to the electrode.

6. The apparatus of claim 5, wherein the infusion medium source is saline.
7. The apparatus of claim 1, further comprising:  
an insulation sleeve positioned in a surrounding relationship to at least a  
5 portion of an exterior surface of the electrode.
8. The apparatus of claim 1, further comprising:  
a sensor positioned at a distal end of the electrode.
9. The apparatus of claim 7, further comprising:  
a first sensor positioned at a distal end of the electrode and a second  
10 sensor positioned at a distal end of the insulation sleeve.
10. The apparatus of claim 1, further comprising:  
a sensor positioned at an exterior surface of the electrode.
11. The apparatus of claim 8, further comprising:  
a sensor positioned at a distal end of the insulation sleeve.
12. The apparatus of claim 1, further comprising:  
a sensor positioned at the catheter tissue interface surface.
13. The apparatus of claim 1, wherein the electrode is coupled to a  
RF energy source.
14. The apparatus of claim 1, wherein the electrode is coupled to a  
20 microwave energy source.

15. The apparatus of claim 1, wherein the electrode is advanced into an interior of a tongue through a ventral surface of the tongue.

16. The apparatus of claim 1, wherein the electrode is advanced into an interior of a tongue through an inferior dorsal surface of the tongue.

5 17. The apparatus of claim 1, wherein the electrode is advanced into an interior of a tongue through a dorsum surface of the tongue.

18. The apparatus of claim 1, wherein two or more electrodes are each advanced into a different interior region of a tongue.

10 19. An apparatus for ablating at least a portion of an interior of a body structure, comprising:

a catheter including a catheter interior, a catheter distal end, a catheter proximal end, a catheter tissue interface surface and a port formed in the catheter;

15 an electrode at least partially positioned in the interior of the catheter and configured to be advanced and retracted to and from the port into an interior of the body structure to deliver sufficient electromagnetic energy to debulk a portion of the interior of the body structure;

20 means for cooling at least a portion of the catheter tissue interface surface sufficiently to reduce a swelling of an exterior surface of the body structure following a delivery of electromagnetic energy to the interior of the body structure;

an electrode advancement and retraction device at least partially positioned in the interior of the catheter; and

a cable coupled to the electrode.

20. The apparatus of claim 19, wherein at least two electrodes are at least partially positioned in the interior of the catheter and each electrode is deployed through a separate port into the interior of the body structure.

5 21. The apparatus of claim 19, wherein the body structure is the tongue.

22. The apparatus of claim 19, wherein the exterior surface of the body structure is a dorsum surface of the tongue.

23. The apparatus of claim 19, wherein the exterior surface of the body structure is a ventral surface of the tongue.

10 24. The apparatus of claim 19, wherein the exterior surface of the body structure is an inferior dorsal surface of the tongue.

25. The apparatus of claim 19, wherein the means for cooling includes an inlet conduit coupled to a cooling medium source and to an outlet conduit.

15 26. The apparatus of claim 25, wherein the inlet conduit and the outlet conduit form a closed loop in the interior of the catheter.

27. The apparatus of claim 19, further comprising:  
an electromagnetic energy source coupled to the cable.

20 28. The apparatus of claim 27, wherein the electromagnetic energy source is a RF source.

29. The apparatus of claim 19, wherein the means for cooling provides a reduce of a swelling of the exterior surface of a tongue following delivery of electromagnetic energy to an interior of the tongue by at least fifty percent.

5           30. The apparatus of claim 19, wherein the means for cooling provides a reduce of a swelling of the exterior surface of a tongue following delivery of electromagnetic energy to an interior of the tongue by at least seventy-five percent.

10           31. An apparatus for ablating at least a portion of an interior of a tongue, comprising:  
a catheter including a proximal end, a distal end and a catheter tissue interface surface;  
an electrode at least partially positioned in the interior of the catheter and configured to be advanced and retracted in and out of the catheter;  
15           an electrode advancement and retraction device at least partially positioned in the interior of the catheter;  
means for reducing an adenomas response to a surface of the tongue upon delivery of electromagnetic energy to an interior of the tongue by the electrode; and  
20           a cable coupled to the electrode.

32. An apparatus for creating an ablation in an interior of a tongue, comprising:  
a catheter including a proximal end, a distal end and a catheter tissue interface surface;  
25           an electrode at least partially positioned in the interior of the catheter and configured to be advanced and retracted in and out of the catheter through an exterior surface of the tongue, wherein the electrode has a RF energy delivery



surface positioned in the interior of the tongue configured to form an ablation zone in the interior of the tongue;

means for cooling at least a portion of the catheter tissue interface surface and at least a portion of the exterior surface of the tongue while  
5 thermally isolating without cooling the RF energy delivery surface;

an electrode advancement and retraction device at least partially positioned in the interior of the catheter; and

a cable coupled to the electrode.

33. A method for treating airway obstructions, comprising:  
10 providing an ablation apparatus including a catheter with a catheter tissue interface surface, an electrode at least partially positioned in an interior of the catheter and advanceable and retractable to and from the catheter into an interior of a body structure, and a means for cooling the catheter tissue interface surface;

15 advancing the electrode from the interior of the catheter through a body structure external surface into the interior of the body structure;

delivering sufficient energy from the electrode into the interior of the body structure to ablate a portion of the interior of the body structure;

cooling the catheter tissue interface surface sufficiently to reduce a swelling of the body structure external surface; and

20 retracting the electrode from the interior of the body structure.

34. The method of claim 33, wherein the body structure is the tongue.

35. The method of claim 34, wherein the external body surface is a dorsum surface of the tongue.

25 36. The method of claim 34, wherein the exterior body surface is a ventral surface of the tongue.

37. The method of claim 34, wherein the exterior surface is an inferior dorsal surface of the tongue.

38. The method of claim 33, wherein sufficient electromagnetic energy is delivered to an interior of the tongue to ablate at least a portion of the interior of tongue with a minimal ablation of a surface of the tongue.

39. The method of claim 38, wherein a taste buds on the surface of the tongue are not ablated.

40. The method of claim 33, wherein the catheter tissue interface surface is cooled to a temperature of 10 to 30 degrees C.

41. The method of claim 33, wherein at least 1 cm<sup>2</sup> of the catheter tissue interface surface is cooled.

42. The method of claim 33, wherein the ablation apparatus includes two or more electrodes, each advanced and retracted from a separate port formed in the catheter tissue interface surface.

43. The method of claim 34, wherein the interior of the tongue is sufficiently ablated to increase a cross-sectional area of an airway passage.

1/13

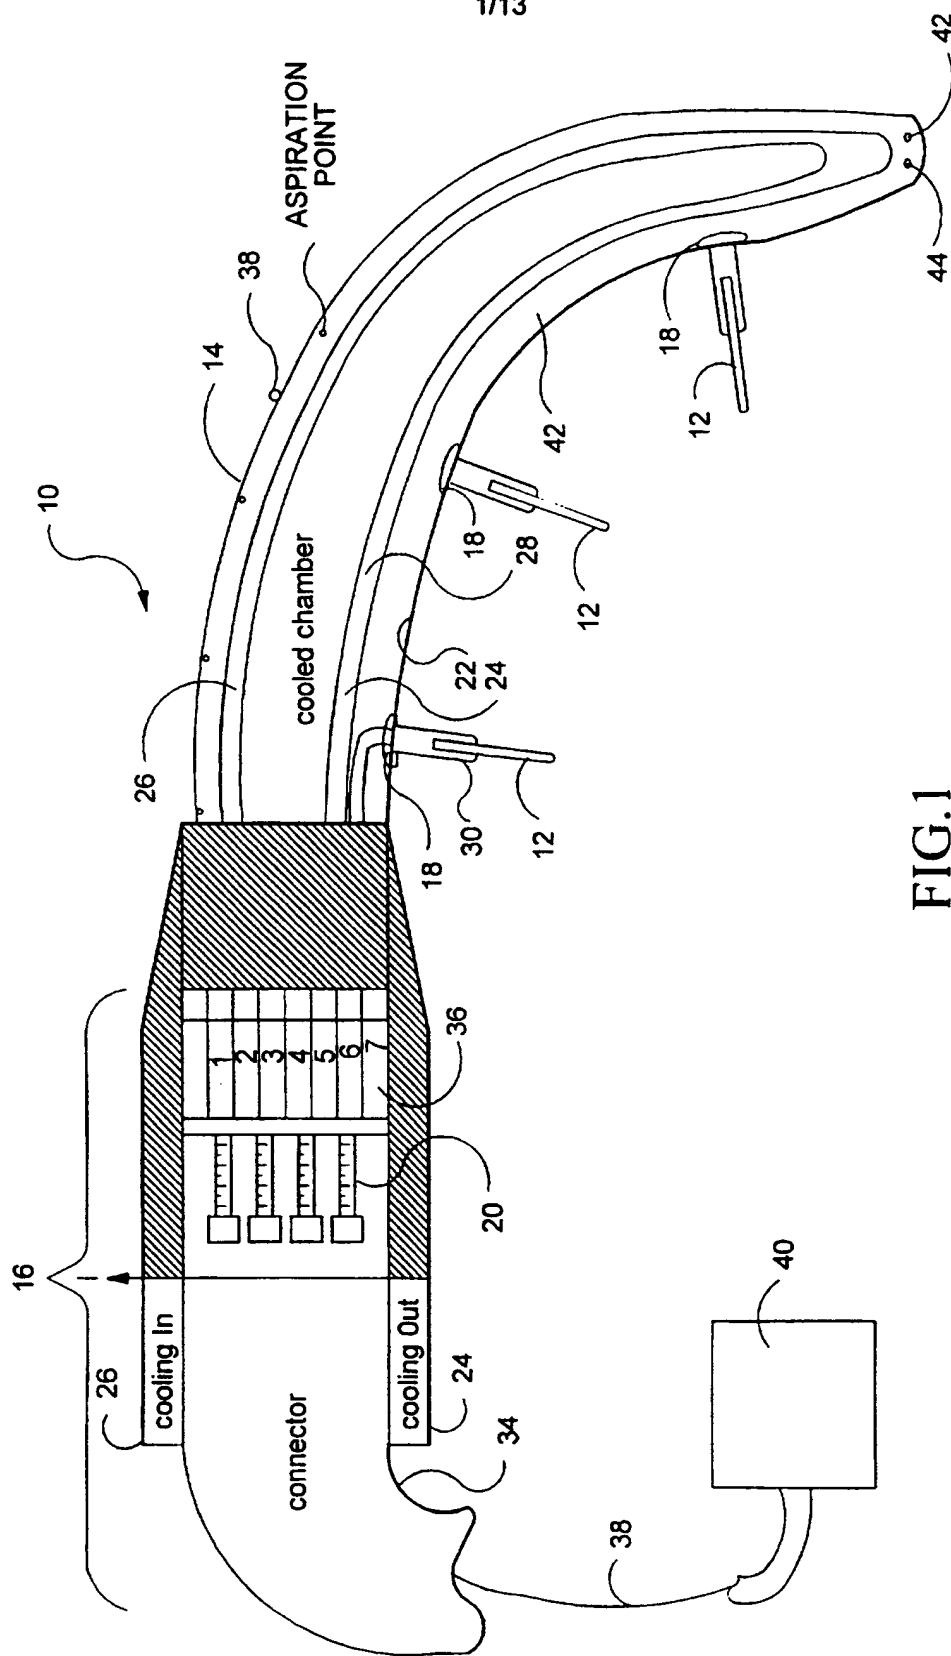


FIG.1

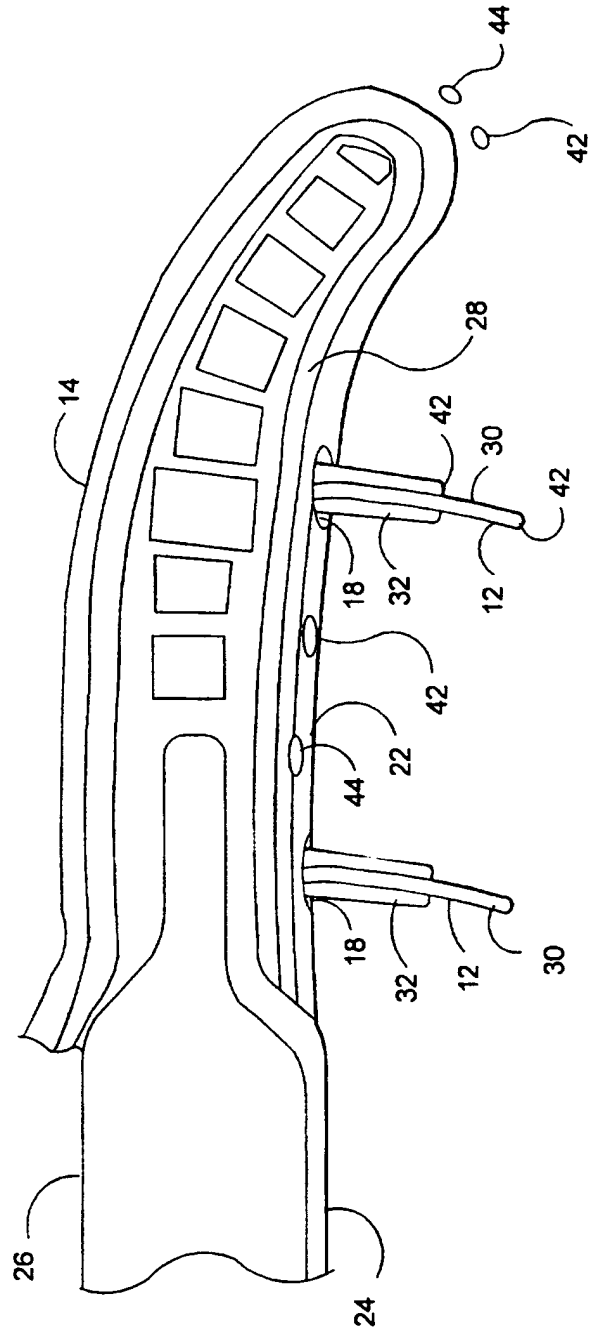


FIG. 2

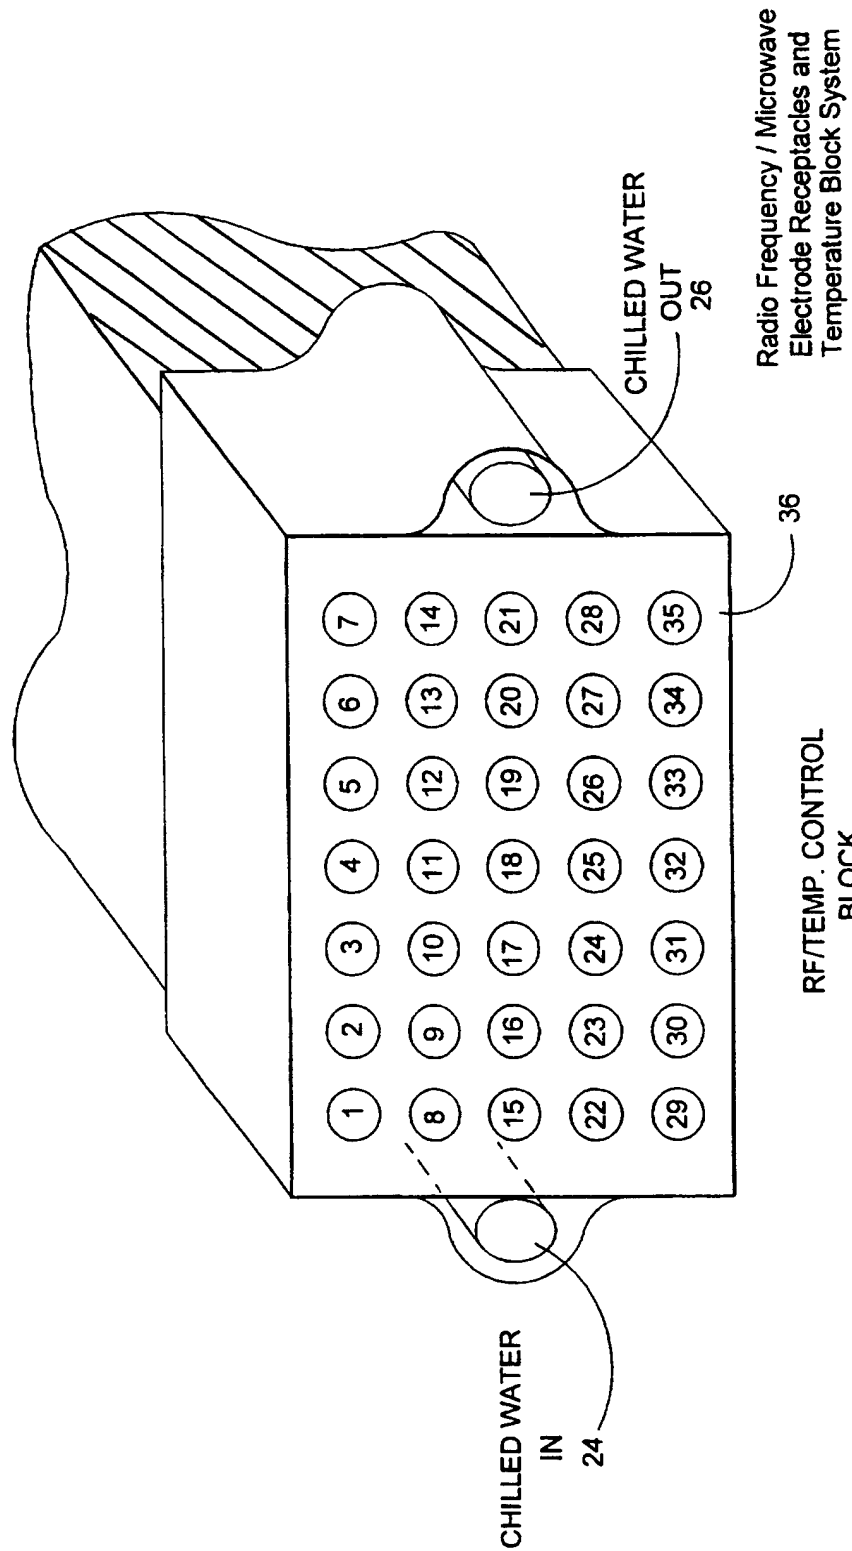


FIG. 3

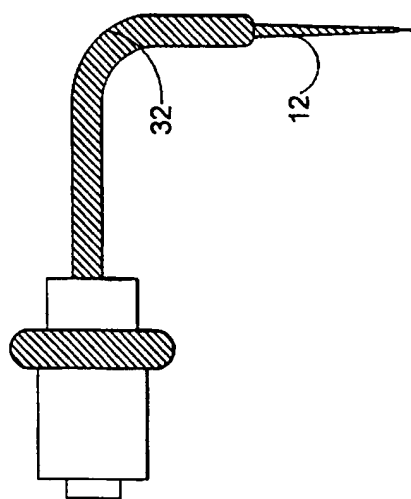


FIG. 5




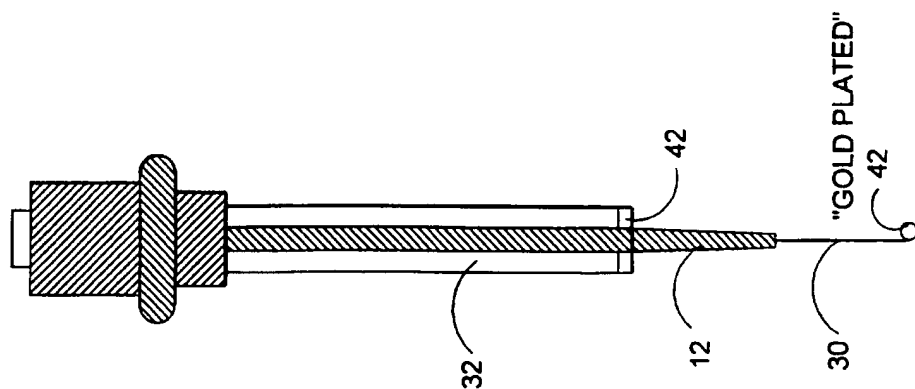


FIG. 4

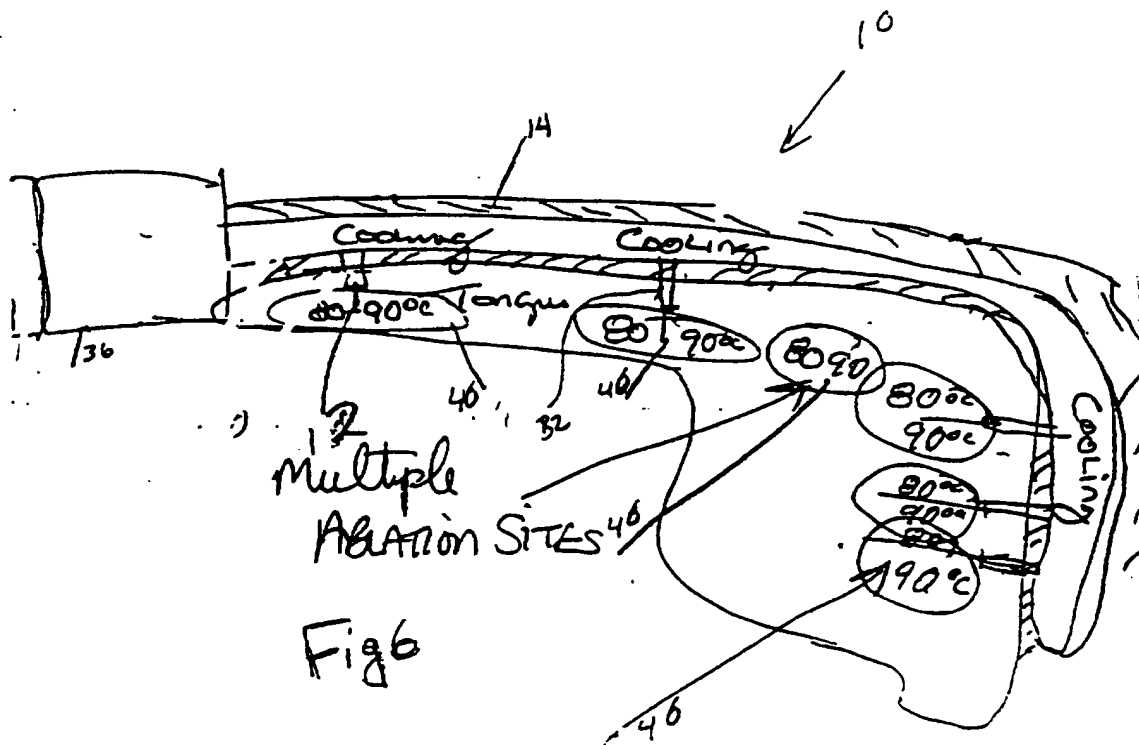

6/13

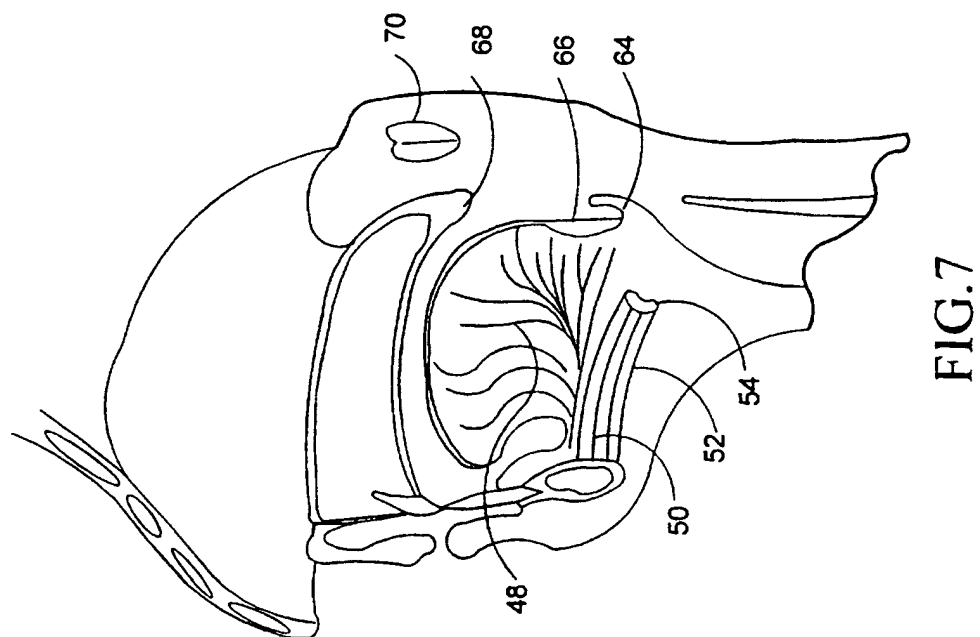

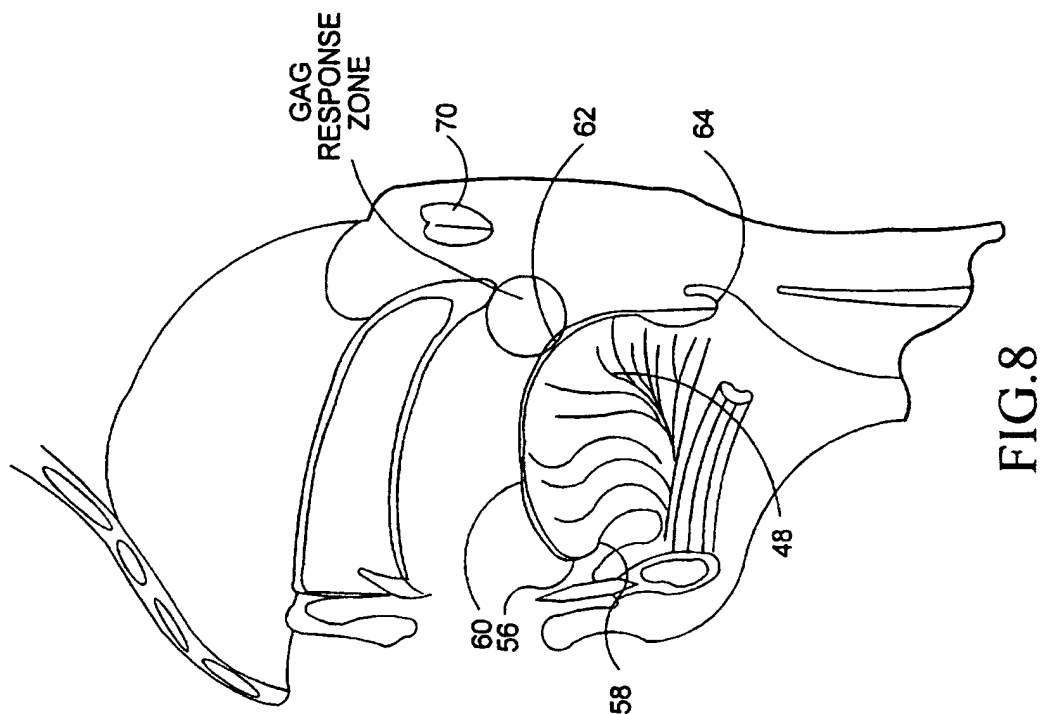

7/13

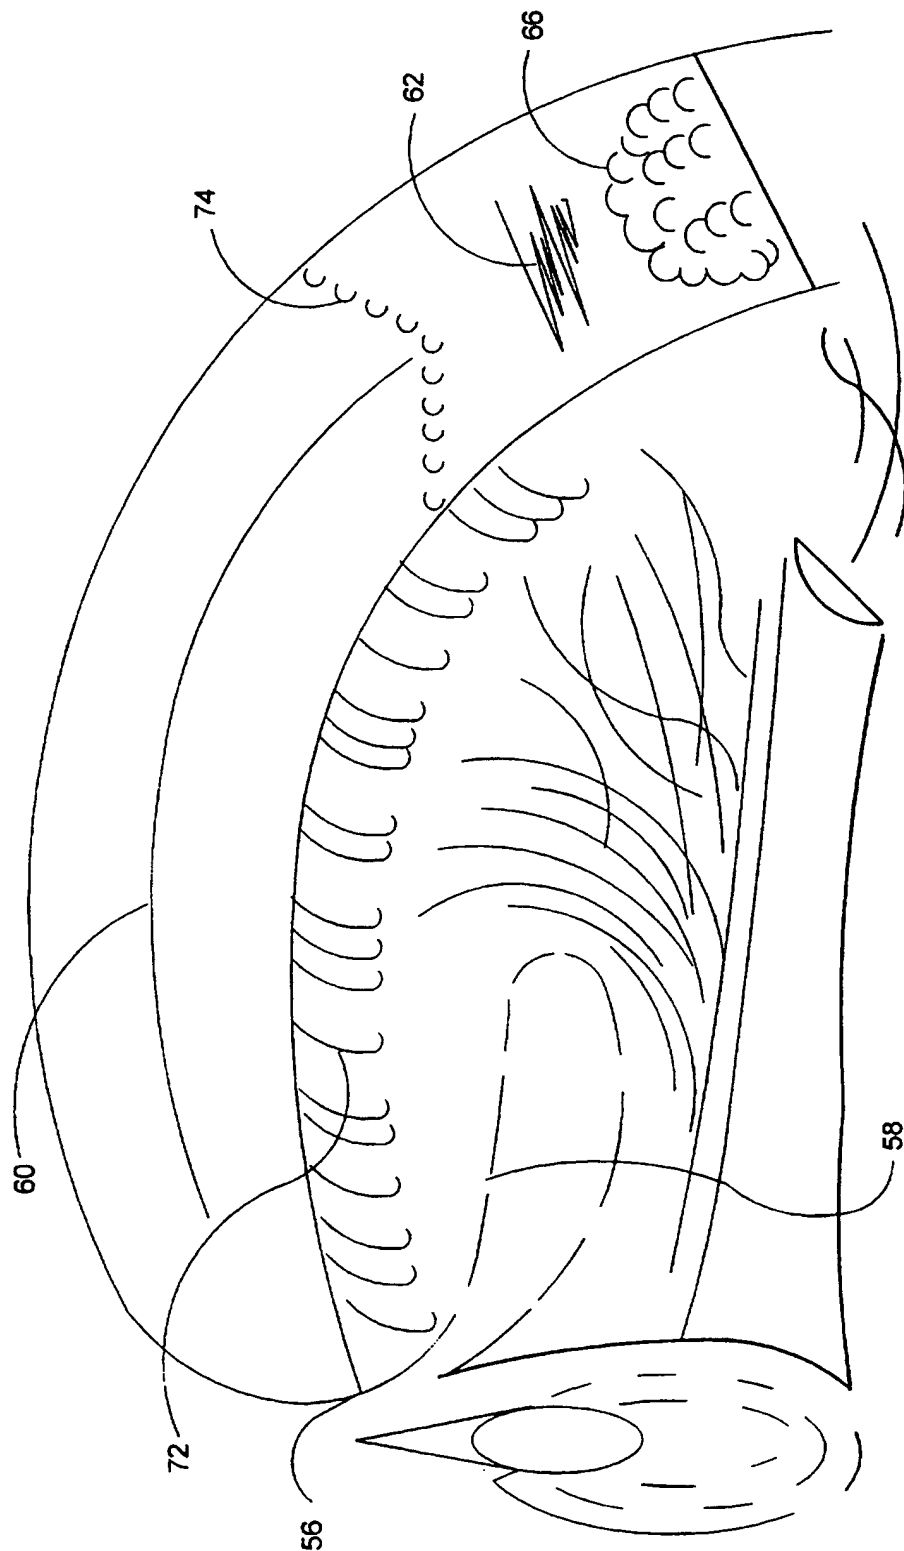


FIG. 9

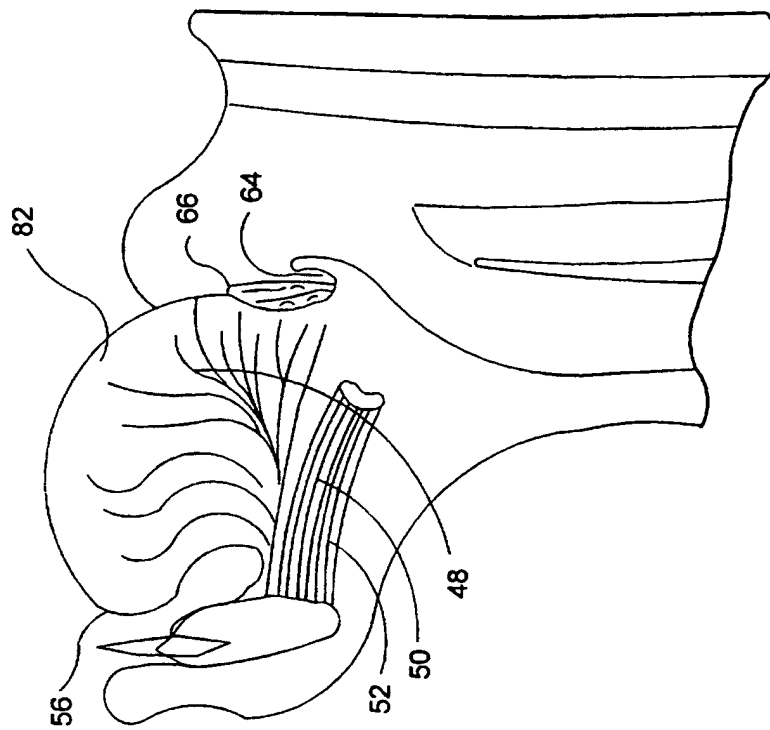


FIG. 11

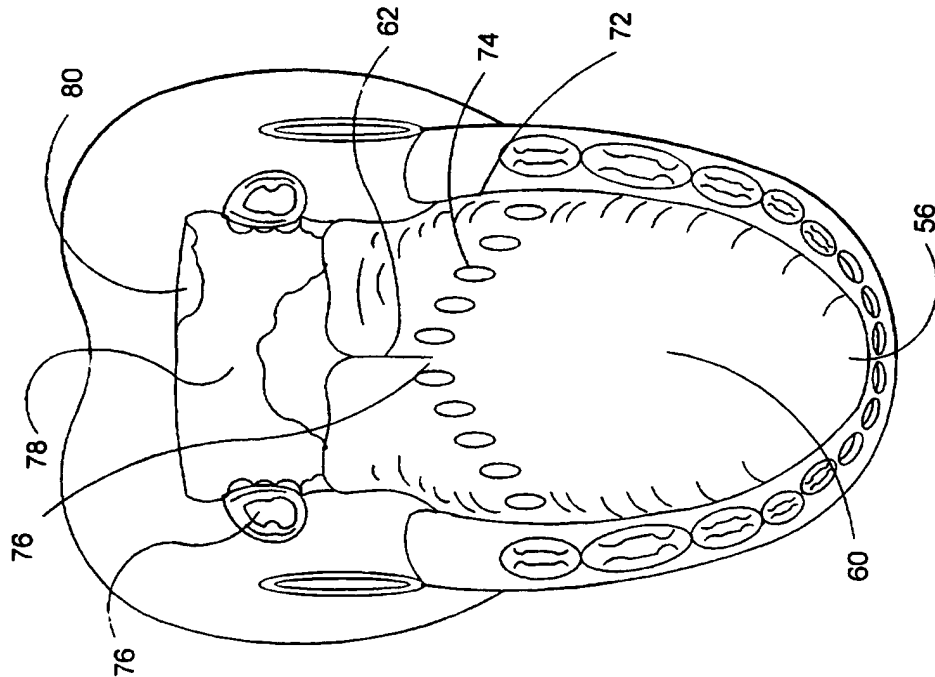


FIG. 10

9/13

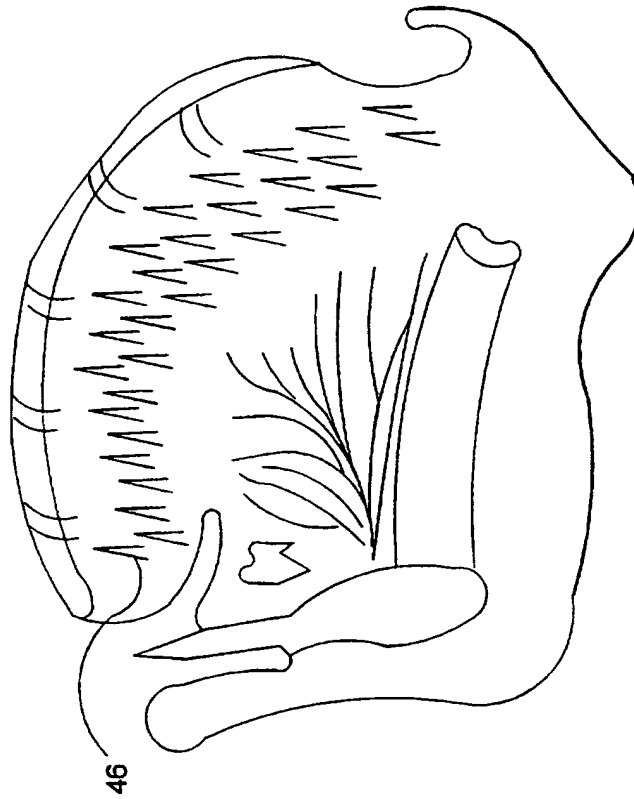


FIG.13

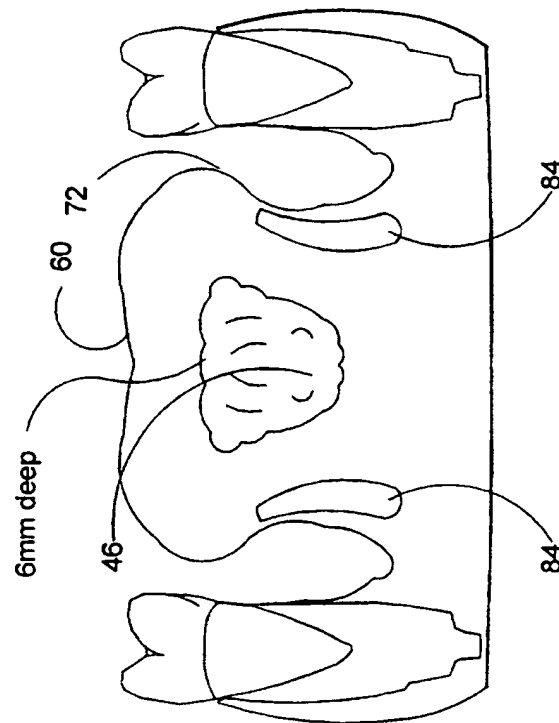


FIG.12

10/13

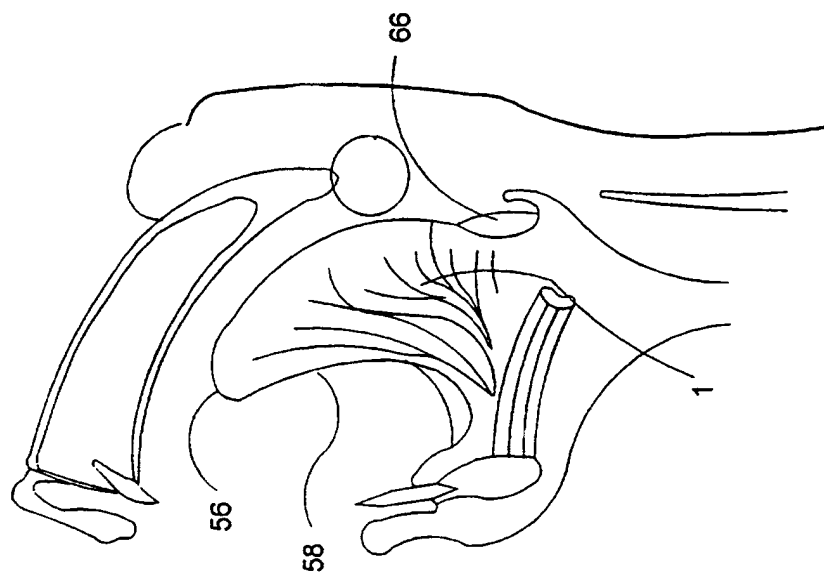


FIG.15

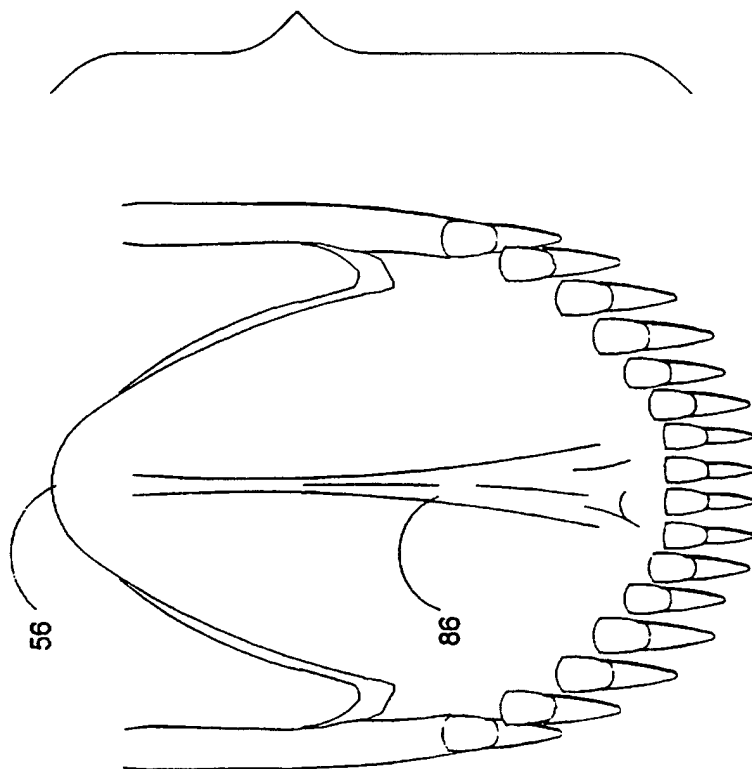


FIG.14

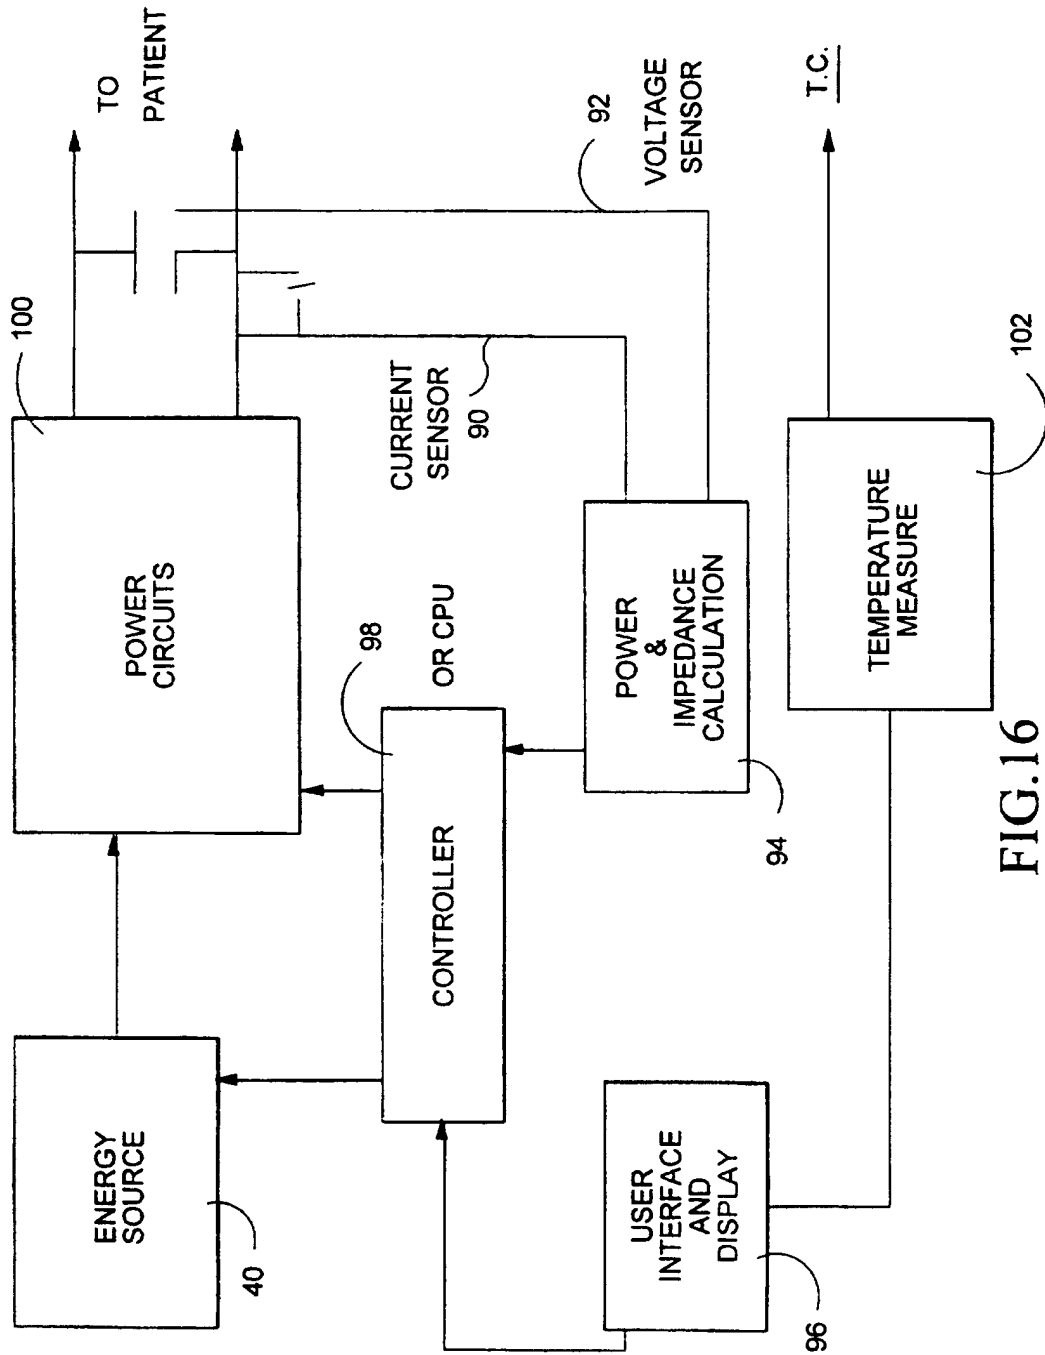


FIG.16

12/13

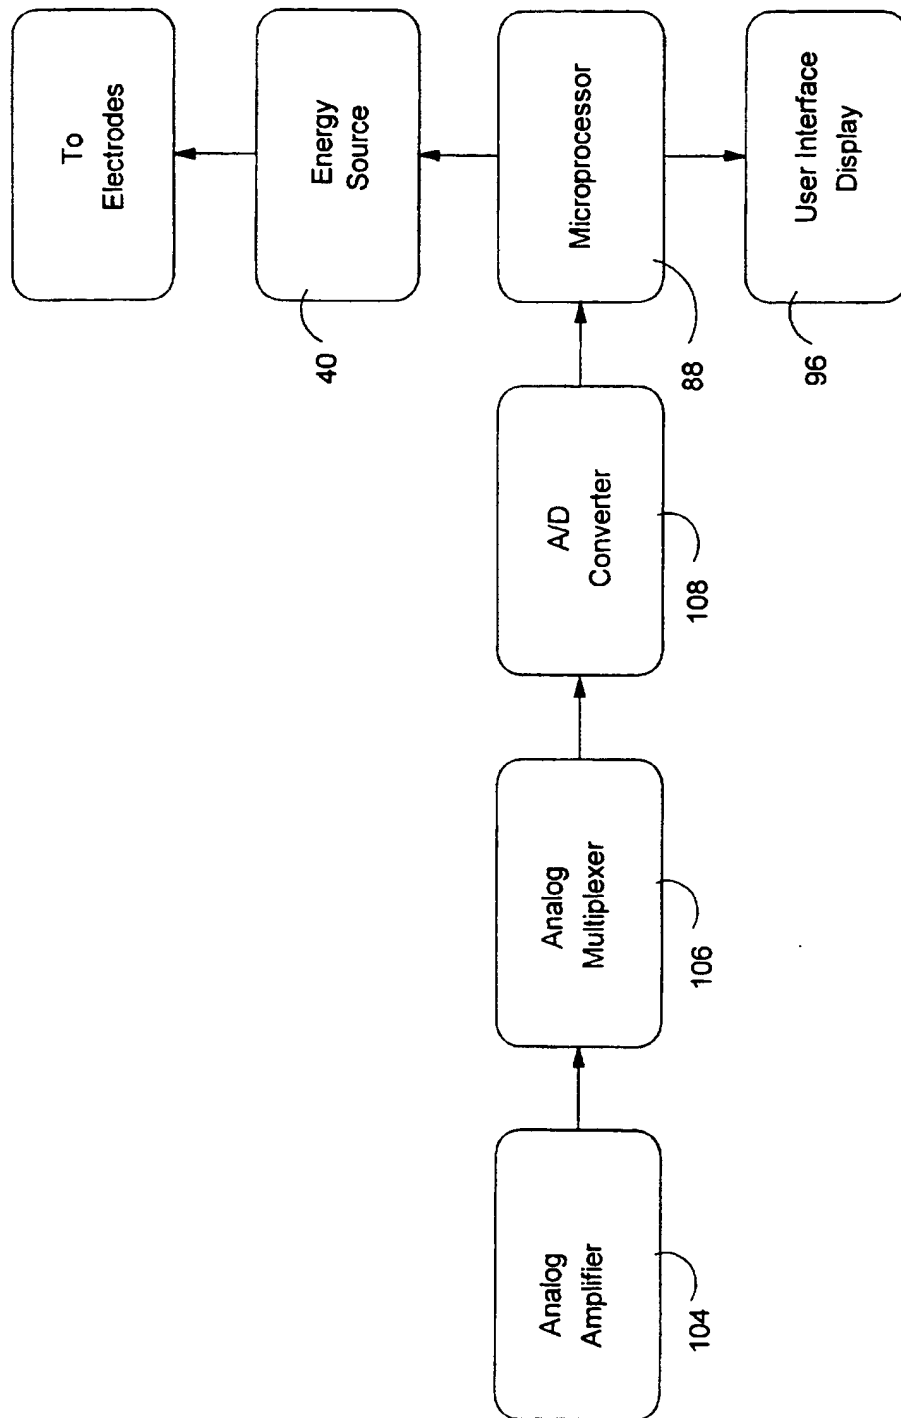


FIG.17

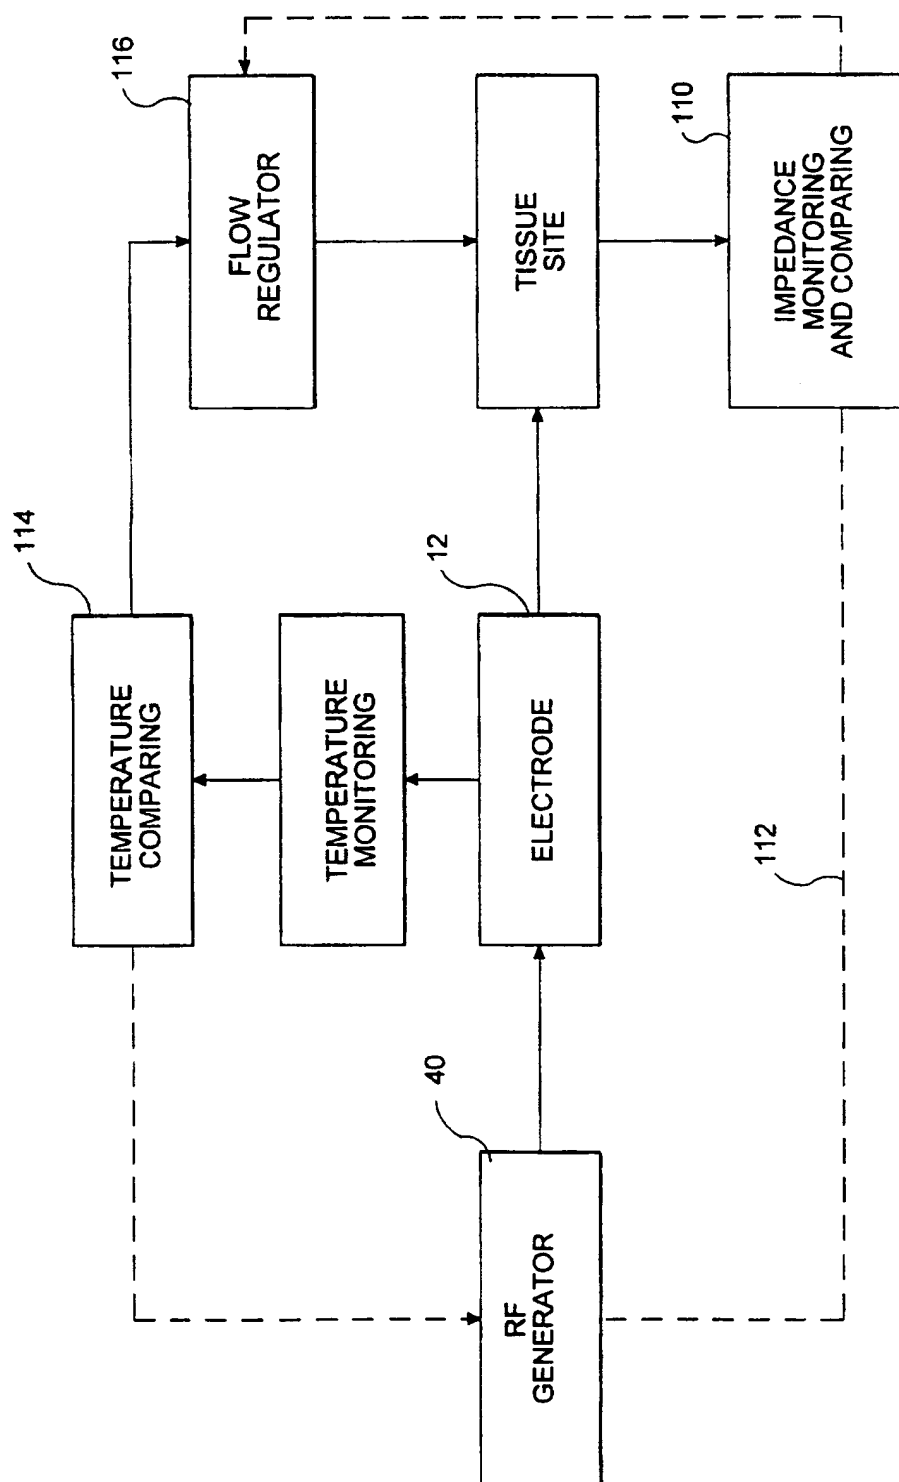


FIG. 18

# INTERNATIONAL SEARCH REPORT

I:      nal Application No  
PCT/US 97/02834

A. CLASSIFICATION OF SUBJECT MATTER  
IPC 6   A61B17/39   A61N1/40   A61N5/04

According to International Patent Classification (IPC) or to both national classification and IPC

## B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)  
IPC 6   A61B   A61N

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practical, search terms used)

## C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	WO 95 18575 A (VIDAMED) 13 July 1995  in partic. page 9 lines 7-9 see the whole document	1,7,14, 31,32
Y	---	4,5,19, 20,25, 26,28
Y	EP 0 608 609 A (CARDIAC PATHWAYS CORP.) 3 August 1994  see column 2, line 22-42 see column 13, paragraph 4	4,5,19, 20,25, 26,28
A	---	3
X	WO 94 26178 A (VIDAMED) 24 November 1994  see the whole document -----	1,7,8, 10,14

☐ Further documents are listed in the continuation of box C.

☒ Patent family members are listed in annex.

### \* Special categories of cited documents:

- \*A\* document defining the general state of the art which is not considered to be of particular relevance
- \*E\* earlier document but published on or after the international filing date
- \*L\* document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)
- \*O\* document referring to an oral disclosure, use, exhibition or other means
- \*P\* document published prior to the international filing date but later than the priority date claimed

- \*T\* later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention
- \*X\* document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone
- \*Y\* document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art.
- \*&\* document member of the same patent family

Date of the actual completion of the international search

17 June 1997

Date of mailing of the international search report

02.07.97

Name and mailing address of the ISA

European Patent Office, P.B. 5818 Patentlaan 2  
NL - 2280 HV Rijswijk  
Tel. (+ 31-70) 340-2040, Tx. 31 651 epo nl,  
Fax (+ 31-70) 340-3016

Authorized officer

Papone, F



# INTERNATIONAL SEARCH REPORT

national application No.

PCT/US 97/ 02834

## Box I Observations where certain claims were found unsearchable (Continuation of item 1 of first sheet)

This International Search Report has not been established in respect of certain claims under Article 17(2)(a) for the following reasons:

1. ☒ Claims Nos.: 33-34  
because they relate to subject matter not required to be searched by this Authority, namely:  
Please see Rule 39.1(iv) PCT
2. ☐ Claims Nos.:  
because they relate to parts of the International Application that do not comply with the prescribed requirements to such an extent that no meaningful International Search can be carried out, specifically:
3. ☐ Claims Nos.:  
because they are dependent claims and are not drafted in accordance with the second and third sentences of Rule 6.4(a).

## Box II Observations where unity of invention is lacking (Continuation of item 2 of first sheet)

This International Searching Authority found multiple inventions in this international application, as follows:

1. ☐ As all required additional search fees were timely paid by the applicant, this International Search Report covers all searchable claims.
2. ☐ As all searchable claims could be searched without effort justifying an additional fee, this Authority did not invite payment of any additional fee.
3. ☐ As only some of the required additional search fees were timely paid by the applicant, this International Search Report covers only those claims for which fees were paid, specifically claims Nos.:
4. ☐ No required additional search fees were timely paid by the applicant. Consequently, this International Search Report is restricted to the invention first mentioned in the claims; it is covered by claims Nos.:

Remark on Protest

- ☐ The additional search fees were accompanied by the applicant's protest.
- ☐ No protest accompanied the payment of additional search fees.

# INTERNATIONAL SEARCH REPORT

information on patent family members

International Application No

PCT/US 97/02834

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
WO 9518575 A	13-07-95	AU 1447695 A US 5599295 A	01-08-95 04-02-97
EP 608609 A	03-08-94	US 5348554 A AU 673015 B AU 5201993 A CA 2110309 A JP 2562861 B JP 6254103 A US 5423811 A US 5545161 A	20-09-94 24-10-96 16-06-94 02-06-94 11-12-96 13-09-94 13-06-95 13-08-96
WO 9426178 A	24-11-94	US 5385544 A AU 6908794 A CN 1128943 A EP 0697837 A JP 8508664 T US 5409453 A US 5486161 A US 5556377 A US 5542915 A US 5484400 A US 5456662 A US 5514131 A US 5542916 A US 5540655 A US 5531677 A US 5599295 A	31-01-95 12-12-94 14-08-96 28-02-96 17-09-96 25-04-95 23-01-96 17-09-96 06-08-96 16-01-96 10-10-95 07-05-96 06-08-96 30-07-96 02-07-96 04-02-97